



**PM500-300 SERIES
LAPTOP PROBE CONNECTIONS**

1. PLUG PROBE'S DB-9 CONNECTOR INTO LAPTOP SERIAL (COM1) PORT
2. VELCRO BATTERY PACK (BP-801) TO LAPTOP LID AS SHOWN
3. PLUG PROBE'S POWER CONNECTOR (PS/2) INTO BATTERY PACK JACK

****NOTE: BATTERY PACK (Picture 2) SHOWN AS OPTIONAL POWER SOURCE FOR PROBE. ONLY NECESSARY WHEN MOUSE (PS/2) PORT NOT AVAILABLE TO CONNECT POWER CONNECTOR (3)**

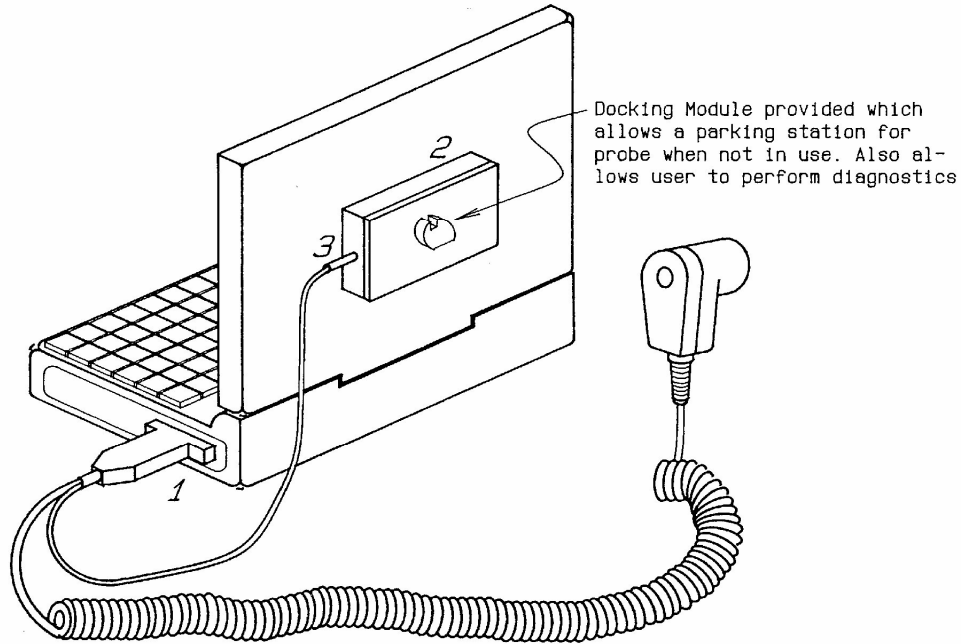

**FOR MODELS PM500-301 OR PM500-308 WITH "DTR" SWITCH
FOR READING SCIENTIFIC COLUMBUS AND JEM METERS**

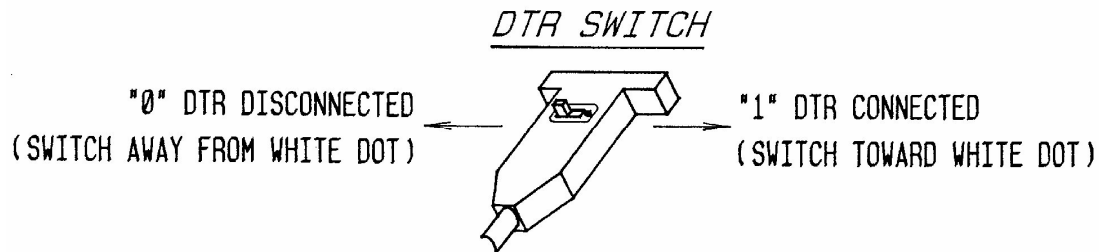

Corporate Office:
uData Net Corp.
6320 Southwest Blvd., Ste. 205
Fort Worth, Texas 76109
(817) 348-9700 Tele
(817) 348-9701 Facsimile
www.udatanet.com

Manufacturing Office:
uData Net Corp.
3247 N. 38th Street
McAllen, Texas 78501
(956) 631-5300 Tele
(956) 631-5193 Facsimile
www.udatanet.com